


Surgical Instruments Catalogue



HOMEDICA
INTERNATIONAL

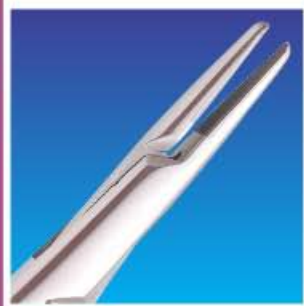

HOMEDICA INTERNATIONAL

Homedica feels great honor introducing itself to be one of the leading manufacturing company of surgical & dental instruments. Professional always prefer Homedica instruments, which is our pride.

Our all instruments are manufactured by the high quality stainless steel made on our requirements, every instrument is hand crafted with the highest workmanship available in the industry. Through heat treatment, the instruments are hardened and tempered for proper functioning and long life. All instruments are polished electrolytically and manually for maximum resistance to corrosion and long life. Homedica pays special attention to the needs of doctors, with innovative designs to meet the needs of professionals. The wide assortment of standard patterns and exclusive Homedica designs gives you the most desirable range of surgical and dental instruments.

Over the several years, we have earned the reputation of for maintaining highest quality standards of quality and service. To manufacture instruments that meet with your changing demands is our achievement. Our highly skilled staff of professionals will continue to serve your needs and will try their outmost to uplift the standards which we have set in the past.

With your co-operation and guidance, Homedica will continue serving surgical and dental instruments in future.

Management of Homedica international

BASIC METHODS FOR HANDLING AND CARE OF SURGICAL AND DENTAL INSTRUMENTS

Dear Customers:

We have received some questions concerning staining, pitting or rusting in stainless steel instruments. So, we took great honour and pleasure in guiding our respected customers to eliminate the problems about staining or rusting etc. The points are as follows:-

- 1) Rinse the instruments as soon as possible after use to remove blood and serum.
- 2) Dry the instruments after cleaning or before wrapping and storing, if not so, moisture left can cause rust and corrosion.
- 3) Do not leave instruments in cold sterilization solution for a long period, as the solution may lead the instrument to be corrosive.
- 4) Never use caustic cleaners, use those specified for cleaning surgical instruments.
- 5) Avoid cleaning instruments with steel wool; if want to clean with hand, use detergent soap and a soft brush and finally treat with distilled water.
- 6) You should check your autoclave; Iron, calcium, sodium or copper in water can cause rusting, staining or corrosion.
- 7) Leaving of instruments for a long time in the following solutions can also cause corrosion.
 - i) Phenol or Iodine.
 - ii) Aluminium, Barium or Calcium.
 - iii) Any Acid, Mercury or Potassium solution.
- 8) Try your utmost not to sterilize stainless steel instrument with chrome plated brass instruments, as any break in chrome surface may cause pitting or rusty surface in instruments.
- 9) Muslin wraps should be rinsed sufficiently by the laundry, so that all chlorine bleach may remove, which can cause corrosion or custing during autoclaving.

We hope that by acting on the above instructions, your problems relating to rusting, staining or pitting would abolish and the age of your instrument would increase.

MANAGEMENT

TROCARS, SUCTION TUBES & CANNULAS



TROCARS

Trokare | Trócares
Trocartes | Tre quarti



UNIVERSAL Abdominal Trocar Set
HI-02-001
(Handle with 4 needles) 14 cm, 5 1/2"
Fig. 1.7 mm Ø to 6 mm Ø
HI-02-002
Only Handle

UNIVERSAL Abdominal Trocar Set
HI-02-007
(Handle with 4 needles) 14 cm, 5 1/2"
Fig. 1.7 mm Ø to 6 mm Ø
HI-02-008
Only Handle




LUER, Trocar
HI-02-013
Luer Lock Adapter



UCKERMANN, Trocar
HI-02-014
13.0 cm 5"



SINUSCOPY, Trocar
17.0 cm 6 3/4"

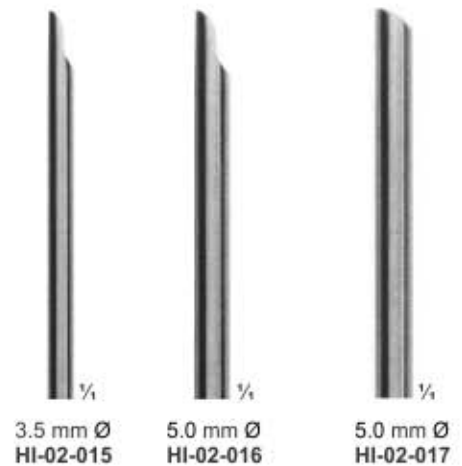



Complete
HI-02-018 1.8 mm Ø
HI-02-019 2.0 mm Ø

LICHTWITZ
Antrum Trocar
19 cm, 7 1/2"




HI-02-020 3 1/3 mm Ø
HI-02-021 4 mm Ø
HI-02-022 4 2/3 mm Ø
HI-02-023 5 1/3 mm Ø
HI-02-024 6 mm Ø
HI-02-025 6 2/3 mm Ø
HI-02-026 7 1/3 mm Ø
HI-02-027 8 mm Ø
HI-02-028 8 2/3 mm Ø
HI-02-029 9 1/3 mm Ø

OCHSNER
Trocar Thorax
10.0 cm 4"




NELSON
Trocar Thorax
21.0 cm 8 1/4"

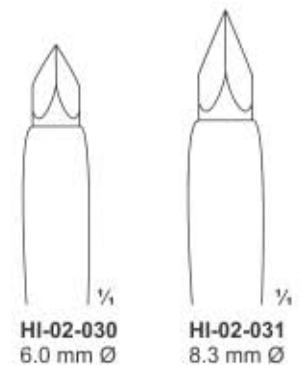

HI-02-030
6.0 mm Ø

HI-02-031
8.3 mm Ø

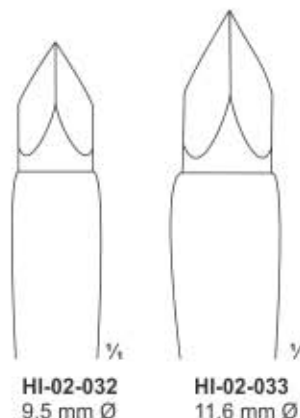

HI-02-032
9.5 mm Ø

HI-02-033
11.6 mm Ø



LANDAU, Trocar
HI-02-034 2.0 mm Ø
16 cm 6 1/4"



HI-02-035 3.0 mm Ø
HI-02-036 4.0 mm Ø
HI-02-037 5.0 mm Ø

PIERCE
Antrum Trocar
17.0 cm 6 3/4"



KRAUSE, Trocar
HI-02-038 15.0 cm 6"
5.5 mm Ø



COAKLEY, Trocar
HI-02-039 16.0 cm 6 1/4"
2.25 mm Ø

SUCTION TUBES



Saugrohre | Tubos de aspiración
 Canules d'aspiration | Tubi per aspirazione



ADSON
 Suction Tubes
HI-02-040
 4 mm Ø
 15 cm, 6"



ADSON
 Suction Tubes
 21.0 cm 8 1/4"
HI-02-041 4 mm Ø 12 Charr./Fr.
HI-02-042 5 mm Ø 15 Charr./Fr.



PLESTER
 Suction Tubes
 17.0 cm 6 3/4"



FERGUSON
 Suction Tubes
 17.0 cm 6 3/4"

| | | | | | |
|------------------|------------|---------------|------------------|------------|---------------|
| HI-02-043 | 2 mm Ø | 6 Charr./Fr. | HI-02-051 | 2 mm Ø | 6 Charr./Fr. |
| HI-02-044 | 2 1/3 mm Ø | 7 Charr./Fr. | HI-02-052 | 2 1/3 mm Ø | 7 Charr./Fr. |
| HI-02-045 | 2 2/3 mm Ø | 8 Charr./Fr. | HI-02-053 | 2 2/3 mm Ø | 8 Charr./Fr. |
| HI-02-046 | 3 mm Ø | 9 Charr./Fr. | HI-02-054 | 3 mm Ø | 9 Charr./Fr. |
| HI-02-047 | 3 1/3 mm Ø | 10 Charr./Fr. | HI-02-055 | 3 1/3 mm Ø | 10 Charr./Fr. |
| HI-02-048 | 3 2/3 mm Ø | 11 Charr./Fr. | HI-02-056 | 3 2/3 mm Ø | 11 Charr./Fr. |
| HI-02-049 | 4 mm Ø | 12 Charr./Fr. | HI-02-057 | 4 mm Ø | 12 Charr./Fr. |
| HI-02-050 | 5 mm Ø | 15 Charr./Fr. | HI-02-058 | 5 mm Ø | 15 Charr./Fr. |



Yankauer
 suction tube
HI-02-059
 27.0 cm, 10 3/4"



FRAZIER
 Suction Tubes
HI-02-060 6 Fr.
HI-02-061 7 Fr.
HI-02-062 9 Fr.
HI-02-063 11 Fr.
 19 cm, 7 1/2"



FRAZIER 30°
 Suction Tubes
HI-02-064 6 Fr.
HI-02-065 7 Fr.
HI-02-066 8 Fr.
HI-02-067 9 Fr.
HI-02-068 10 Fr.
HI-02-069 11 Fr.
HI-02-070 12 Fr.
HI-02-071 15 Fr.
 18 cm, 7"



FRAZIER 45°
 Suction Tubes
HI-02-072 6 Fr.
HI-02-073 7 Fr.
HI-02-074 8 Fr.
HI-02-075 9 Fr.
HI-02-076 10 Fr.
HI-02-077 11 Fr.
HI-02-078 12 Fr.
 18 cm, 7"



HARTMANN,
Eustachian Catheters
Fig. 1
HI-02-079 2.0 mm Ø
HI-02-080 2.5 mm Ø
HI-02-081 3.0 mm Ø



HARTMANN
Eustachian Catheters
Fig. 2
HI-02-082 2.0 mm Ø
HI-02-083 2.5 mm Ø
HI-02-084 3.0 mm Ø



KILLIAN, Eustachian Catheters
HI-02-085 16.0 cm 6" 2.5 mm Ø
HI-02-086 16.0 cm 6" 3.0 mm Ø
oval opening



Fig. 0
HI-02-087

Fig. 2
HI-02-089

Fig. 4
HI-02-091

HARTMANN
Eustachian Catheters
15.0 cm 6"



Fig. 1
HI-02-088



Fig. 3
HI-02-090



Fig. 5
HI-02-092



TRÖLTSCHE
Eustachian Catheters
15.0 cm 6"



HI-02-093
Tube end piece
for eustachian
catheter



Fig. 2
HI-02-095



Fig. 4
HI-02-097



Fig. 1
HI-02-094



Fig. 3
HI-02-096



Fig. 5
HI-02-098

SUCTION TUBES, GUIDE NEEDLE



Saugrohre, Redon Führungsnadeln

Tubos para aspiración, Agujas de guía

Tubes d'aspiration, Aiguilles d'introduction

Cannule d'aspirazione, Aghi guida



ZÖLLNER, Suction Tube
HI-02-099 0.7 mm Ø
 complete with 1 slip-on
 cannula, 0.7 mm Ø



IOWA, Suction Tube
HI-02-100 0.7 mm Ø
 16.0 cm 6 1/4"



MAGILL, Suction Tube
 24.5 cm 9 3/4"
HI-02-101 3.0 mm Ø
HI-02-102 3.5 mm Ø
HI-02-103 4.0 mm Ø



ROSEN, Suction Tube
 X=80 mm
HI-02-104 0.7 mm Ø
HI-02-105 0.9 mm Ø
HI-02-106 1.2 mm Ø



ROSEN, Suction Tube
 X=65 mm
HI-02-107 0.7 mm Ø
HI-02-108 0.9 mm Ø
HI-02-109 1.2 mm Ø



SUCTION TUBE, Guide Needle
 19.5 cm 5 3/4"
HI-02-110 2.2/3 mm Ø 8 Charr./Fr.
HI-02-111 3.1/3 mm Ø 10 Charr./Fr.
HI-02-112 4 mm Ø 12 Charr./Fr.
HI-02-113 4 2/3 mm Ø 14 Charr./Fr.
HI-02-114 5 1/3 mm Ø 16 Charr./Fr.
HI-02-115 6 mm Ø 18 Charr./Fr.



SUCTION TUBE, Guide Needle
 19.5 cm 5 3/4"
HI-02-116 2 mm Ø 6 Charr./Fr.
HI-02-117 2.2/3 mm Ø 8 Charr./Fr.
HI-02-118 3 1/3 mm Ø 10 Charr./Fr.
HI-02-119 4 mm Ø 12 Charr./Fr.
HI-02-120 4 2/3 mm Ø 14 Charr./Fr.
HI-02-121 5 1/3 mm Ø 16 Charr./Fr.
HI-02-122 6 1/3 mm Ø 18 Charr./Fr.



SUCTION TUBE, Guide Needle
Lancet Tip 19.5 cm 5 3/4"
HI-02-123 2.2/3 mm Ø 8 Charr./Fr.
HI-02-124 3.1/3 mm Ø 10 Charr./Fr.
HI-02-125 4 mm Ø 12 Charr./Fr.
HI-02-126 4 2/3 mm Ø 14 Charr./Fr.
HI-02-127 5 1/3 mm Ø 16 Charr./Fr.
HI-02-128 6 mm Ø 18 Charr./Fr.

PROBE, Double Ended
2.0 mm Ø

| | |
|-----------|----------------|
| HI-02-129 | 11.5 cm 4 1/2" |
| HI-02-130 | 13.0 cm 5" |
| HI-02-131 | 14.5 cm 5 3/4" |
| HI-02-132 | 16.0 cm 6 1/4" |
| HI-02-133 | 18.0 cm 7" |
| HI-02-134 | 20.0 cm 8" |
| HI-02-135 | 25.0 cm 9 3/4" |

PROBE, Double Ended
1.5 mm Ø

| | |
|-----------|----------------|
| HI-02-136 | 11.5 cm 4 1/2" |
| HI-02-137 | 13.0 cm 5" |
| HI-02-138 | 14.5 cm 5 3/4" |
| HI-02-139 | 16.0 cm 6 1/4" |
| HI-02-140 | 18.0 cm 7" |
| HI-02-141 | 20.0 cm 8" |
| HI-02-142 | 25.0 cm 9 3/4" |

PROBE, Double Ended
1.0 mm Ø

| | |
|-----------|----------------|
| HI-02-143 | 11.5 cm 4 1/2" |
| HI-02-144 | 13.0 cm 5" |
| HI-02-145 | 14.5 cm 5 3/4" |
| HI-02-146 | 16.0 cm 6 1/4" |
| HI-02-147 | 18.0 cm 7" |
| HI-02-148 | 20.0 cm 8" |
| HI-02-149 | 25.0 cm 9 3/4" |

PROBE With Eye

2.0 mm Ø

| | |
|-----------|----------------|
| HI-02-150 | 11.5 cm 4 1/2" |
| HI-02-151 | 13.0 cm 5" |
| HI-02-152 | 14.5 cm 5 3/4" |
| HI-02-153 | 16.0 cm 6 1/4" |
| HI-02-154 | 18.0 cm 7" |
| HI-02-155 | 20.0 cm 8" |
| HI-02-156 | 25.0 cm 9 3/4" |

with eyelet

PROBE

2.0 mm Ø

| | |
|-----------|----------------|
| HI-02-157 | 11.5 cm 4 1/2" |
| HI-02-158 | 13.0 cm 5" |
| HI-02-159 | 14.5 cm 5 3/4" |
| HI-02-160 | 16.0 cm 6 1/4" |

myrtle-shaped



BUTTERFLY GROOVED
Director With Tongue Tie
Plain End

| | |
|-----------|----------------|
| HI-02-161 | 11.5 cm 4 1/2" |
| HI-02-162 | 13.0 cm 5" |
| HI-02-163 | 14.5 cm 5 3/4" |
| HI-02-164 | 16.0 cm 6 1/4" |
| HI-02-165 | 18.0 cm 7" |
| HI-02-166 | 20.0 cm 8" |



BUTTERFLY GROOVED
Director With Tongue Tie
Plain End

| | |
|-----------|----------------|
| HI-02-167 | 11.5 cm 4 1/2" |
| HI-02-168 | 13.0 cm 5" |
| HI-02-169 | 14.5 cm 5 3/4" |
| HI-02-170 | 16.0 cm 6 1/4" |
| HI-02-171 | 18.0 cm 7" |
| HI-02-172 | 20.0 cm 8" |



DOYEN
Probes & Directors
HI-02-173
14.0 cm 5 1/2"



NÉLATON
Probes & Directors
HI-02-174
16.0 cm 6 1/2"

COTTON APPLICATORS



Watteträger | Porta-algodones
 Porte-cotons | Portacotoni



JOPSON-HORNE
 cotton applicator
 HI-02-175
 18.0 cm 7"



FEIN
 cotton applicator
 HI-02-176
 28.0 cm 11"



PELTESON
 cotton applicator
 HI-02-177
 23.0 cm 9"



BARR Fistula Probe
 HI-02-178
 with 8" (20.3 cm) sterling shaft,
 eye at tip, 11-1/2" (29.2 cm) overall



BARR Crypt Hook,
 HI-02-179
 10" (25.4 cm), short and
 long hook ends




BUIE Suction Tube,
 HI-02-180
 18" (45 cm), with finger
 valve, 15 Fr. (5 mm)



Biolvar
 HI-02-181 15cm
 HI-02-182 18cm
 HI-02-183 20cm



Desjardim
 HI-02-184 18cm
 (Set 3 Pieces)

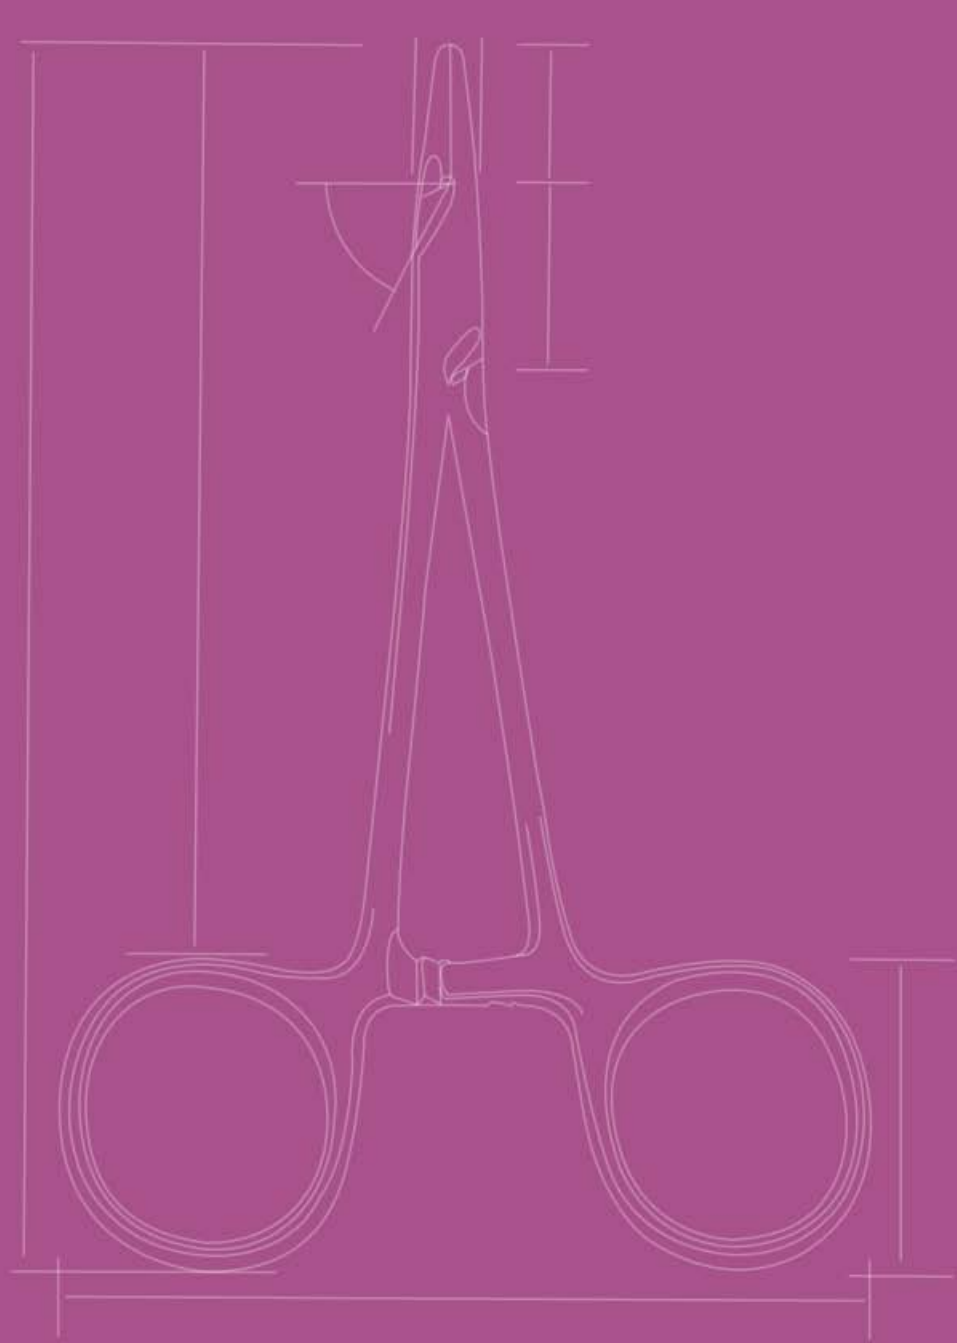

HOMEDICA
INTERNATIONAL